
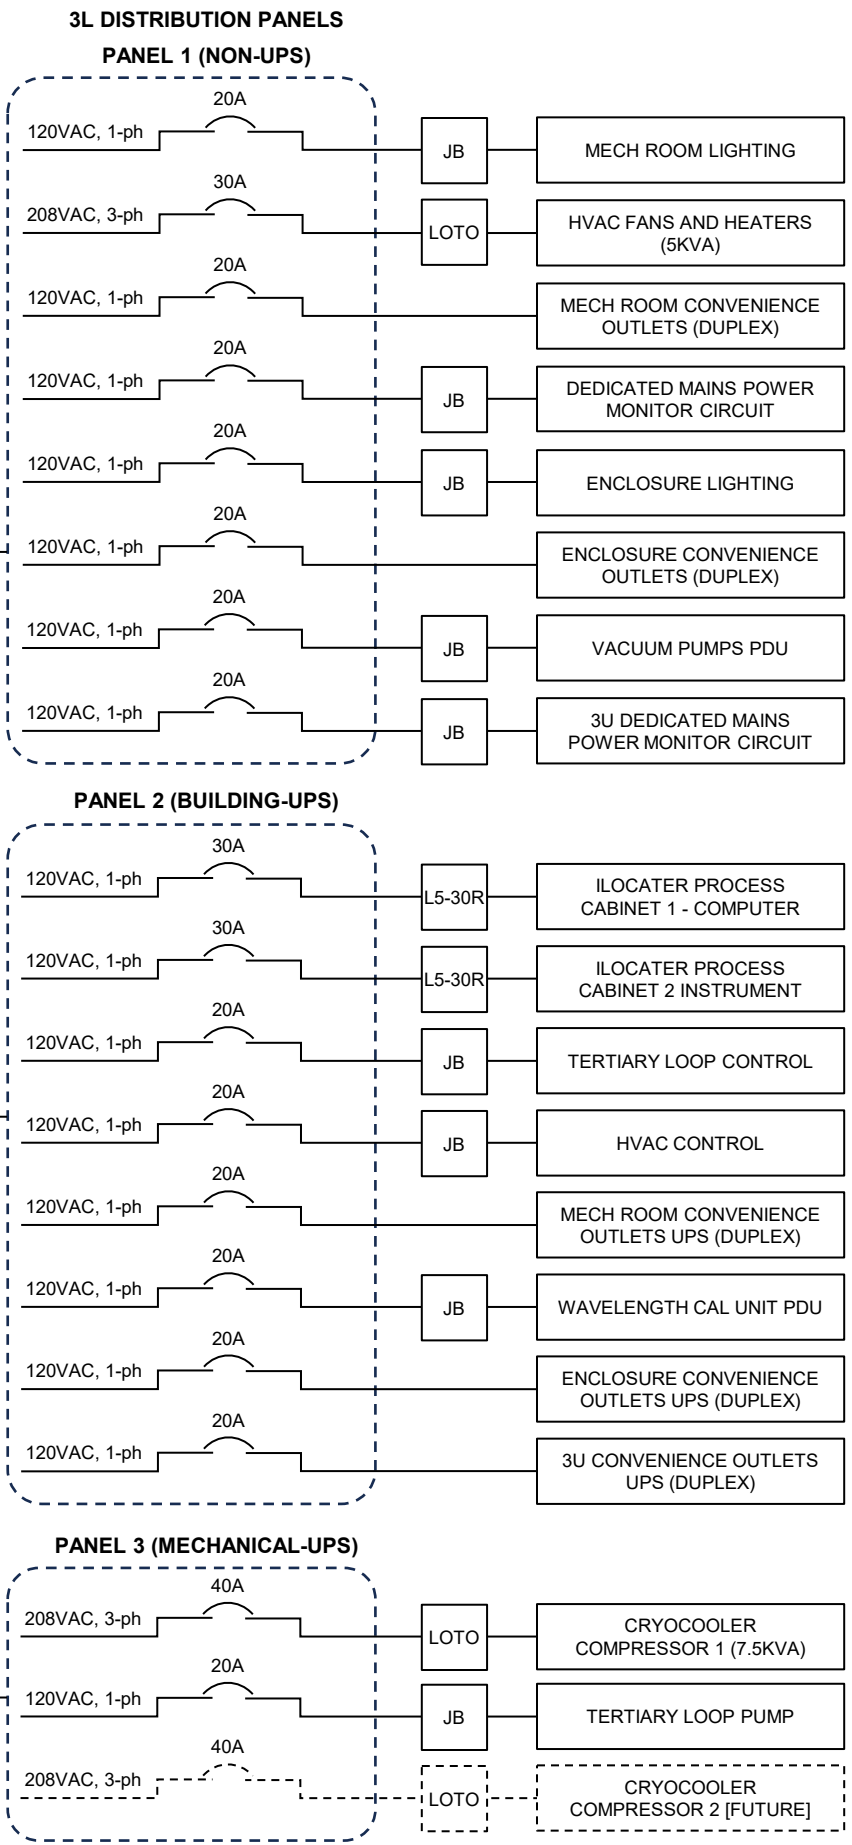


**ILOCATER 3L  
ELECTRICAL DIAGRAM**  
 REV: 7A  
 AUTHOR: J. CRASS  
 DATE: 21 FEB 2024

- JB** JUNCTION BOX
- LOTO** LOCK-OUT/TAG-OUT DISCONNECT
- L5-30R** NEMA L5-30R RECEPTACLE

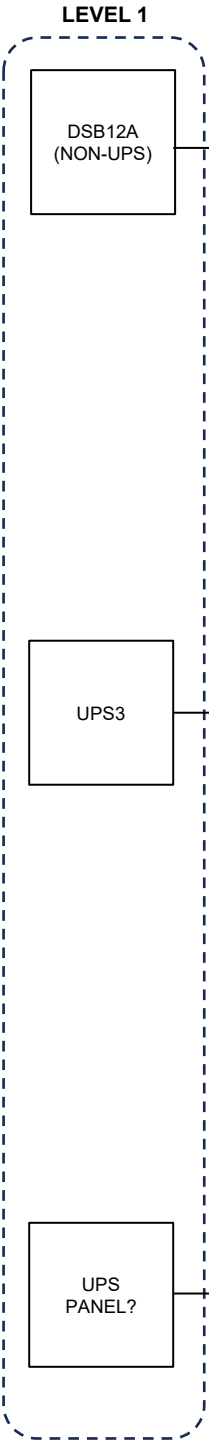

LOADS (A)		
Typical	Operational	Max
0	2	
?	?	?
0	0	10
0	0	0
0	2	
1	1	10
0	6	18
0	0	0
4	4	13.4
		14
?	?	?
3	3	5
0	1	10
		5
0	1	10
0.5	0.5	10
6	6	22
?	?	?
(0)	(6)	(22)